

Fig. 1
1/8


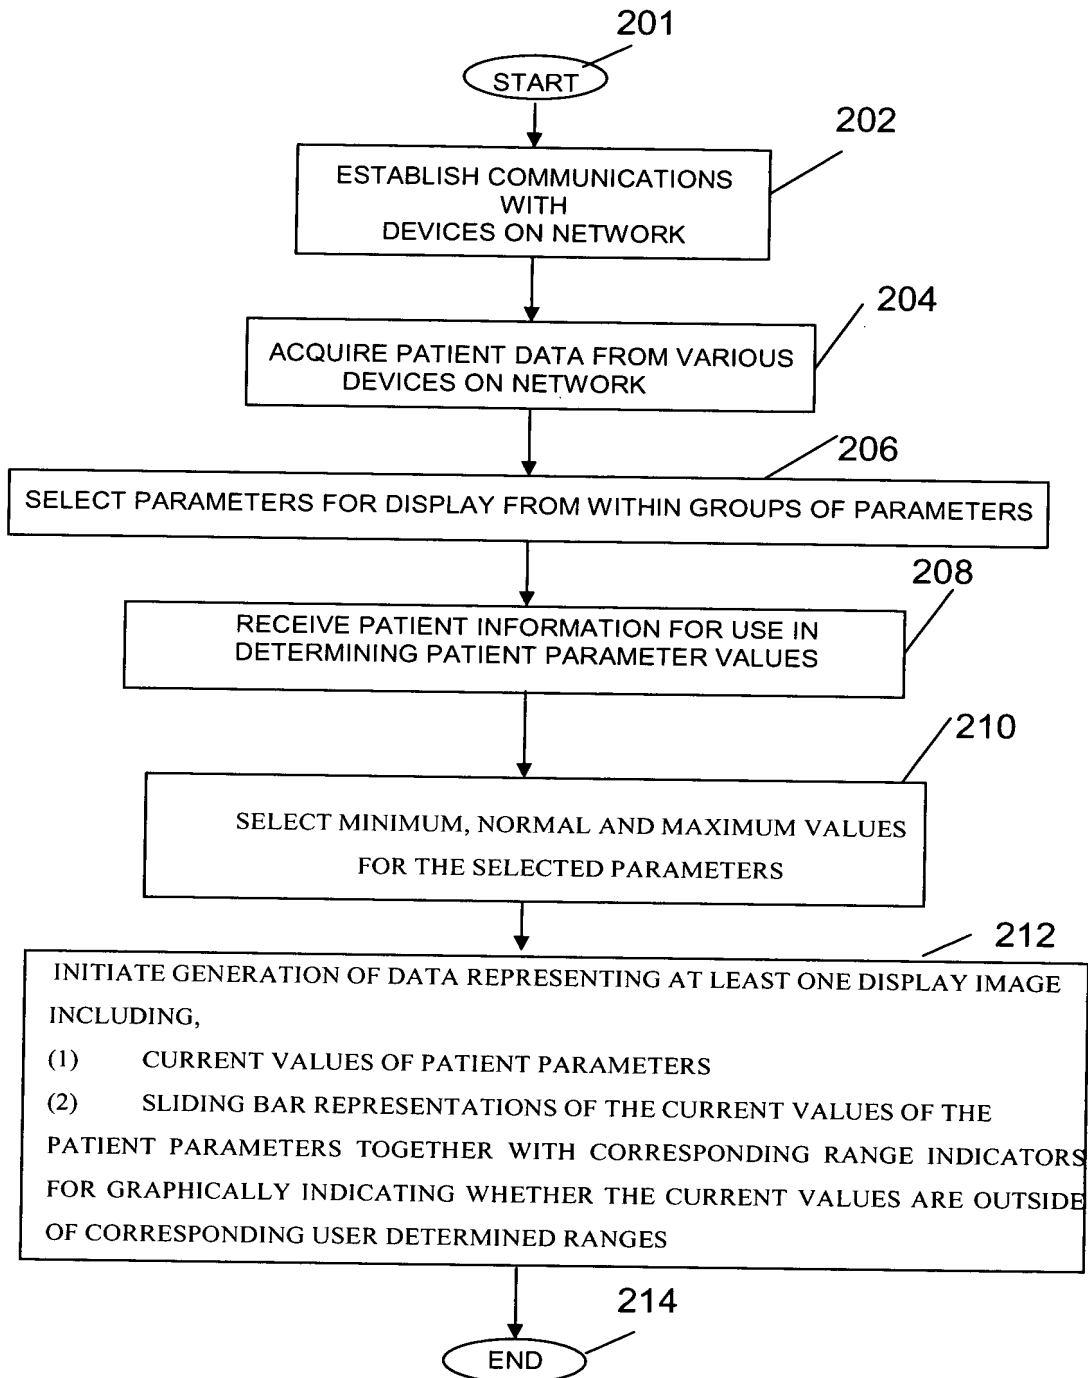


FIGURE 2

3/8
Figure 3

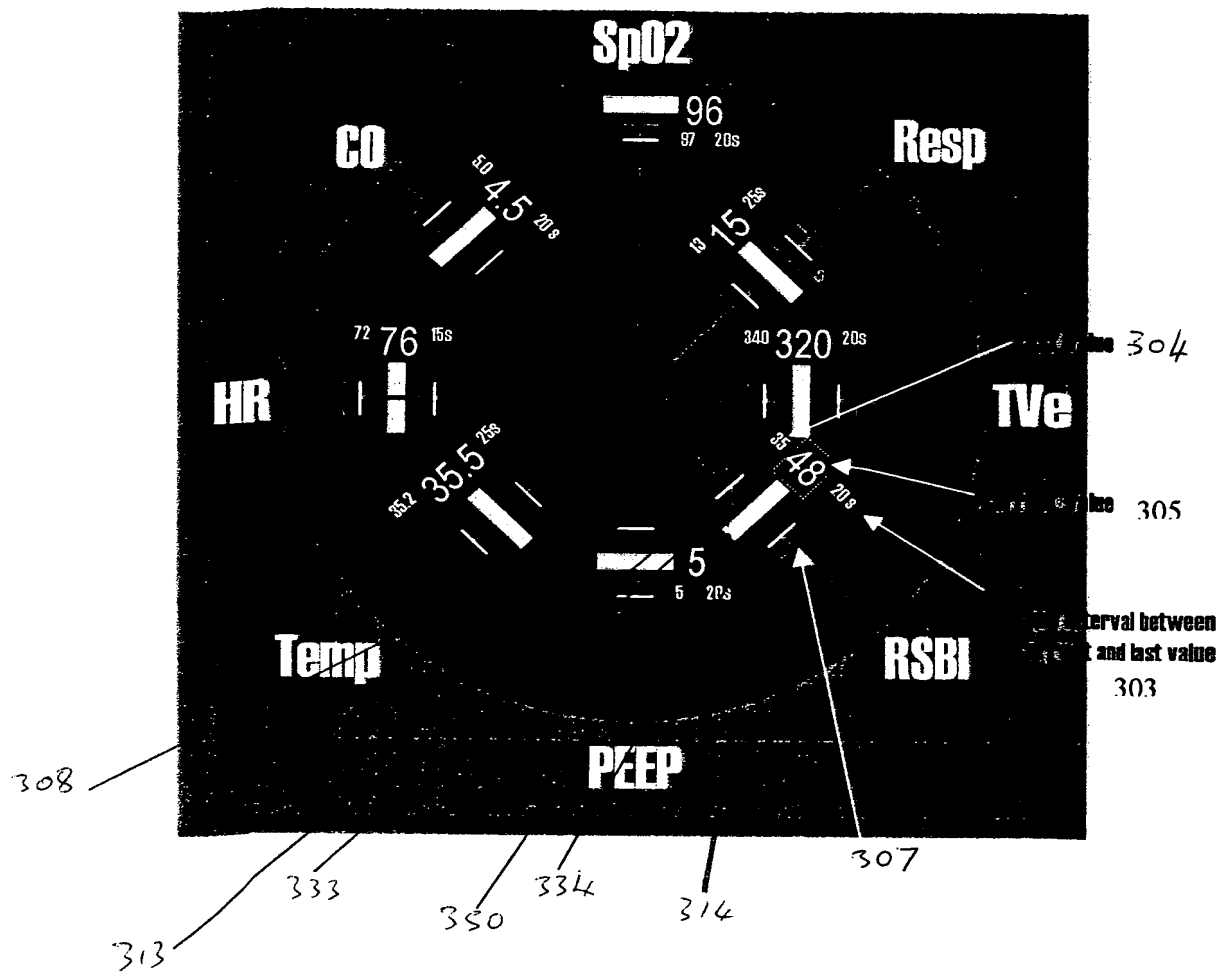

BEST AVAILABLE COPY

400
403
405

Vascular	Respiratory	Laboratory
<input checked="" type="checkbox"/> Pulse	<input checked="" type="checkbox"/> Resp Rate	<input type="checkbox"/> Hemoglobin
<input type="checkbox"/> Cardiac Index	<input checked="" type="checkbox"/> Tidal Volume	<input type="checkbox"/> K
<input checked="" type="checkbox"/> Cardiac Output	<input type="checkbox"/> Minute Volume	<input type="checkbox"/> Ca
<input checked="" type="checkbox"/> O2 Saturation	<input checked="" type="checkbox"/> PEEP	<input type="checkbox"/> SaO2
<input checked="" type="checkbox"/> Core Temp	<input checked="" type="checkbox"/> RSBI	<input type="checkbox"/> PO2
<input type="checkbox"/> PAP	<input type="checkbox"/> IMV Level	<input type="checkbox"/> PCO2
<input type="checkbox"/> CVP	<input type="checkbox"/> Dyn. Compl.	<input type="checkbox"/> pH
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>
<input type="checkbox"/>	<input type="checkbox"/>	<input type="checkbox"/>

407

Selected Parameters
Pulse Cardiac
Output O2
Saturation
Temperature RR
Tve Cardiac Index
Cardiac Index

409
Mass (kg)


53

411
Height (cm)


145

FIGURE 4
4/8

5/8
FIGURE 5

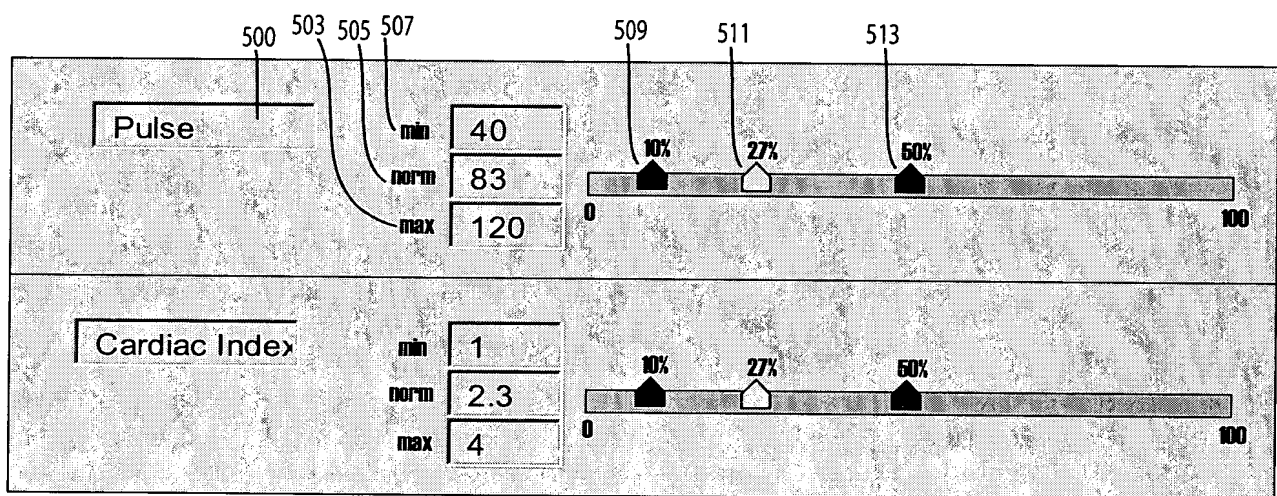


6/8
Figure 6

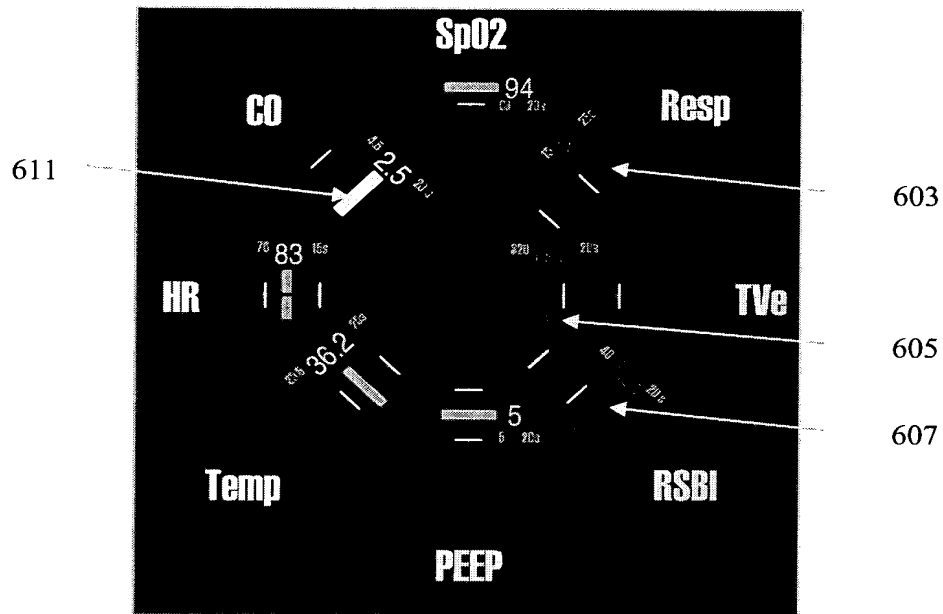

BEST AVAILABLE COPY

7/8
Figure 7

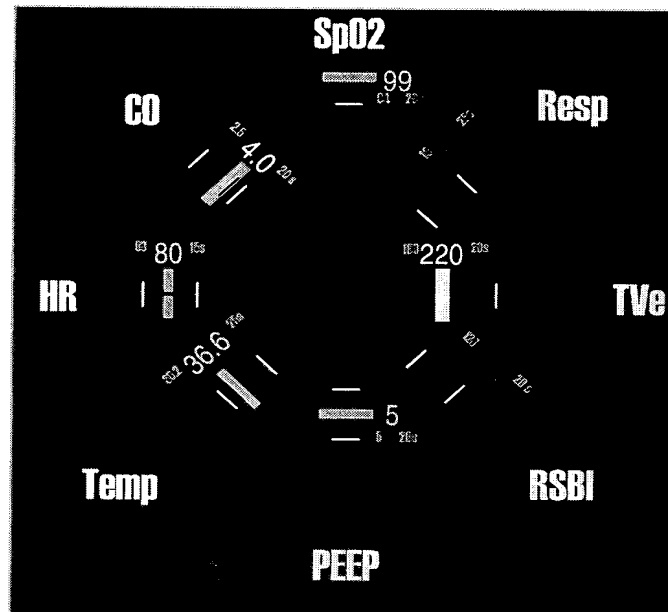

BEST AVAILABLE COPY

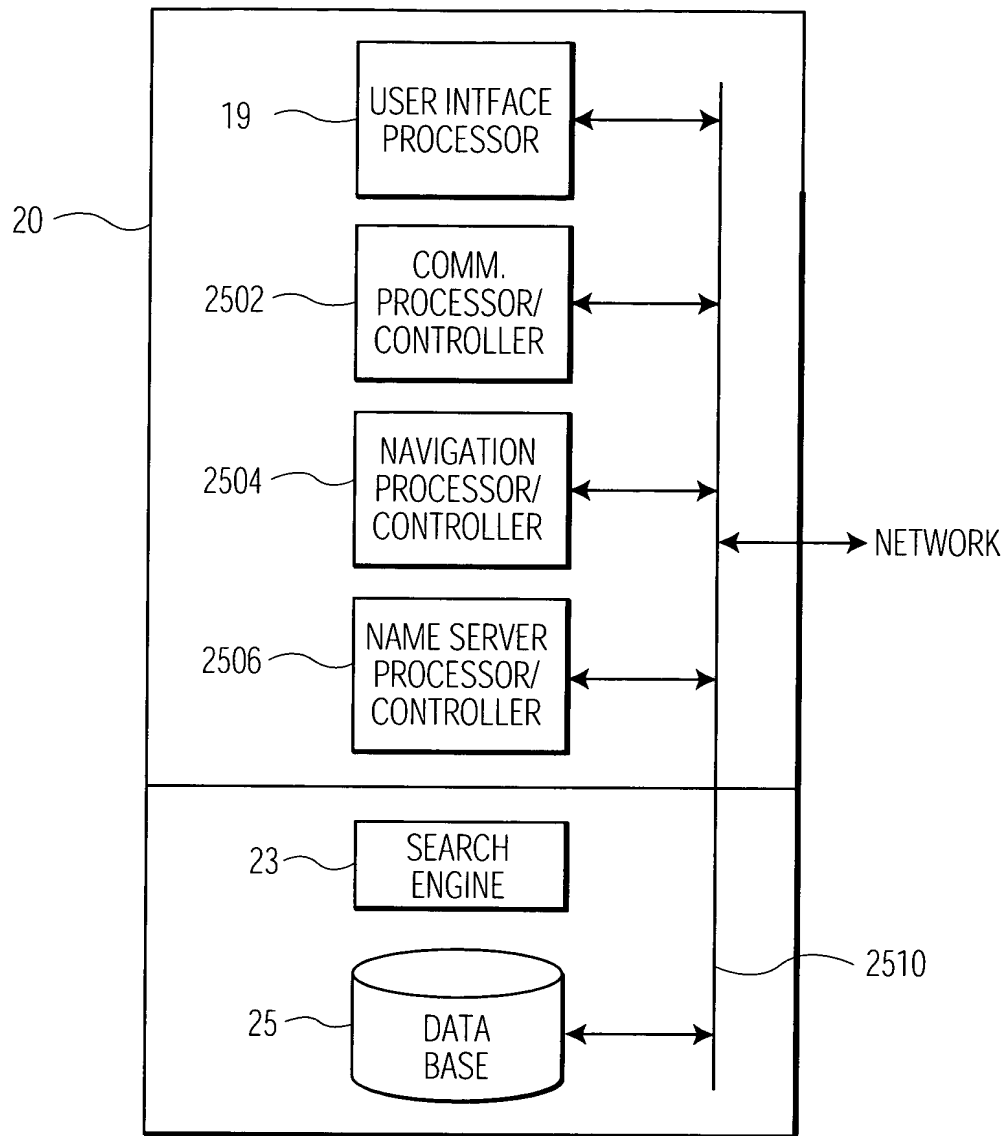


FIGURE 8